PHARMALINE


ONCOLOGY | MICROBIOLOGY | MEDICAL GENETICS

MOLECULAR BIOLOGY RESEARCH AND LABORATORY REAGENTS

PRODUCT CATALOG

2026

www.pharmaline.com.tr I info@pharmaline.com.tr

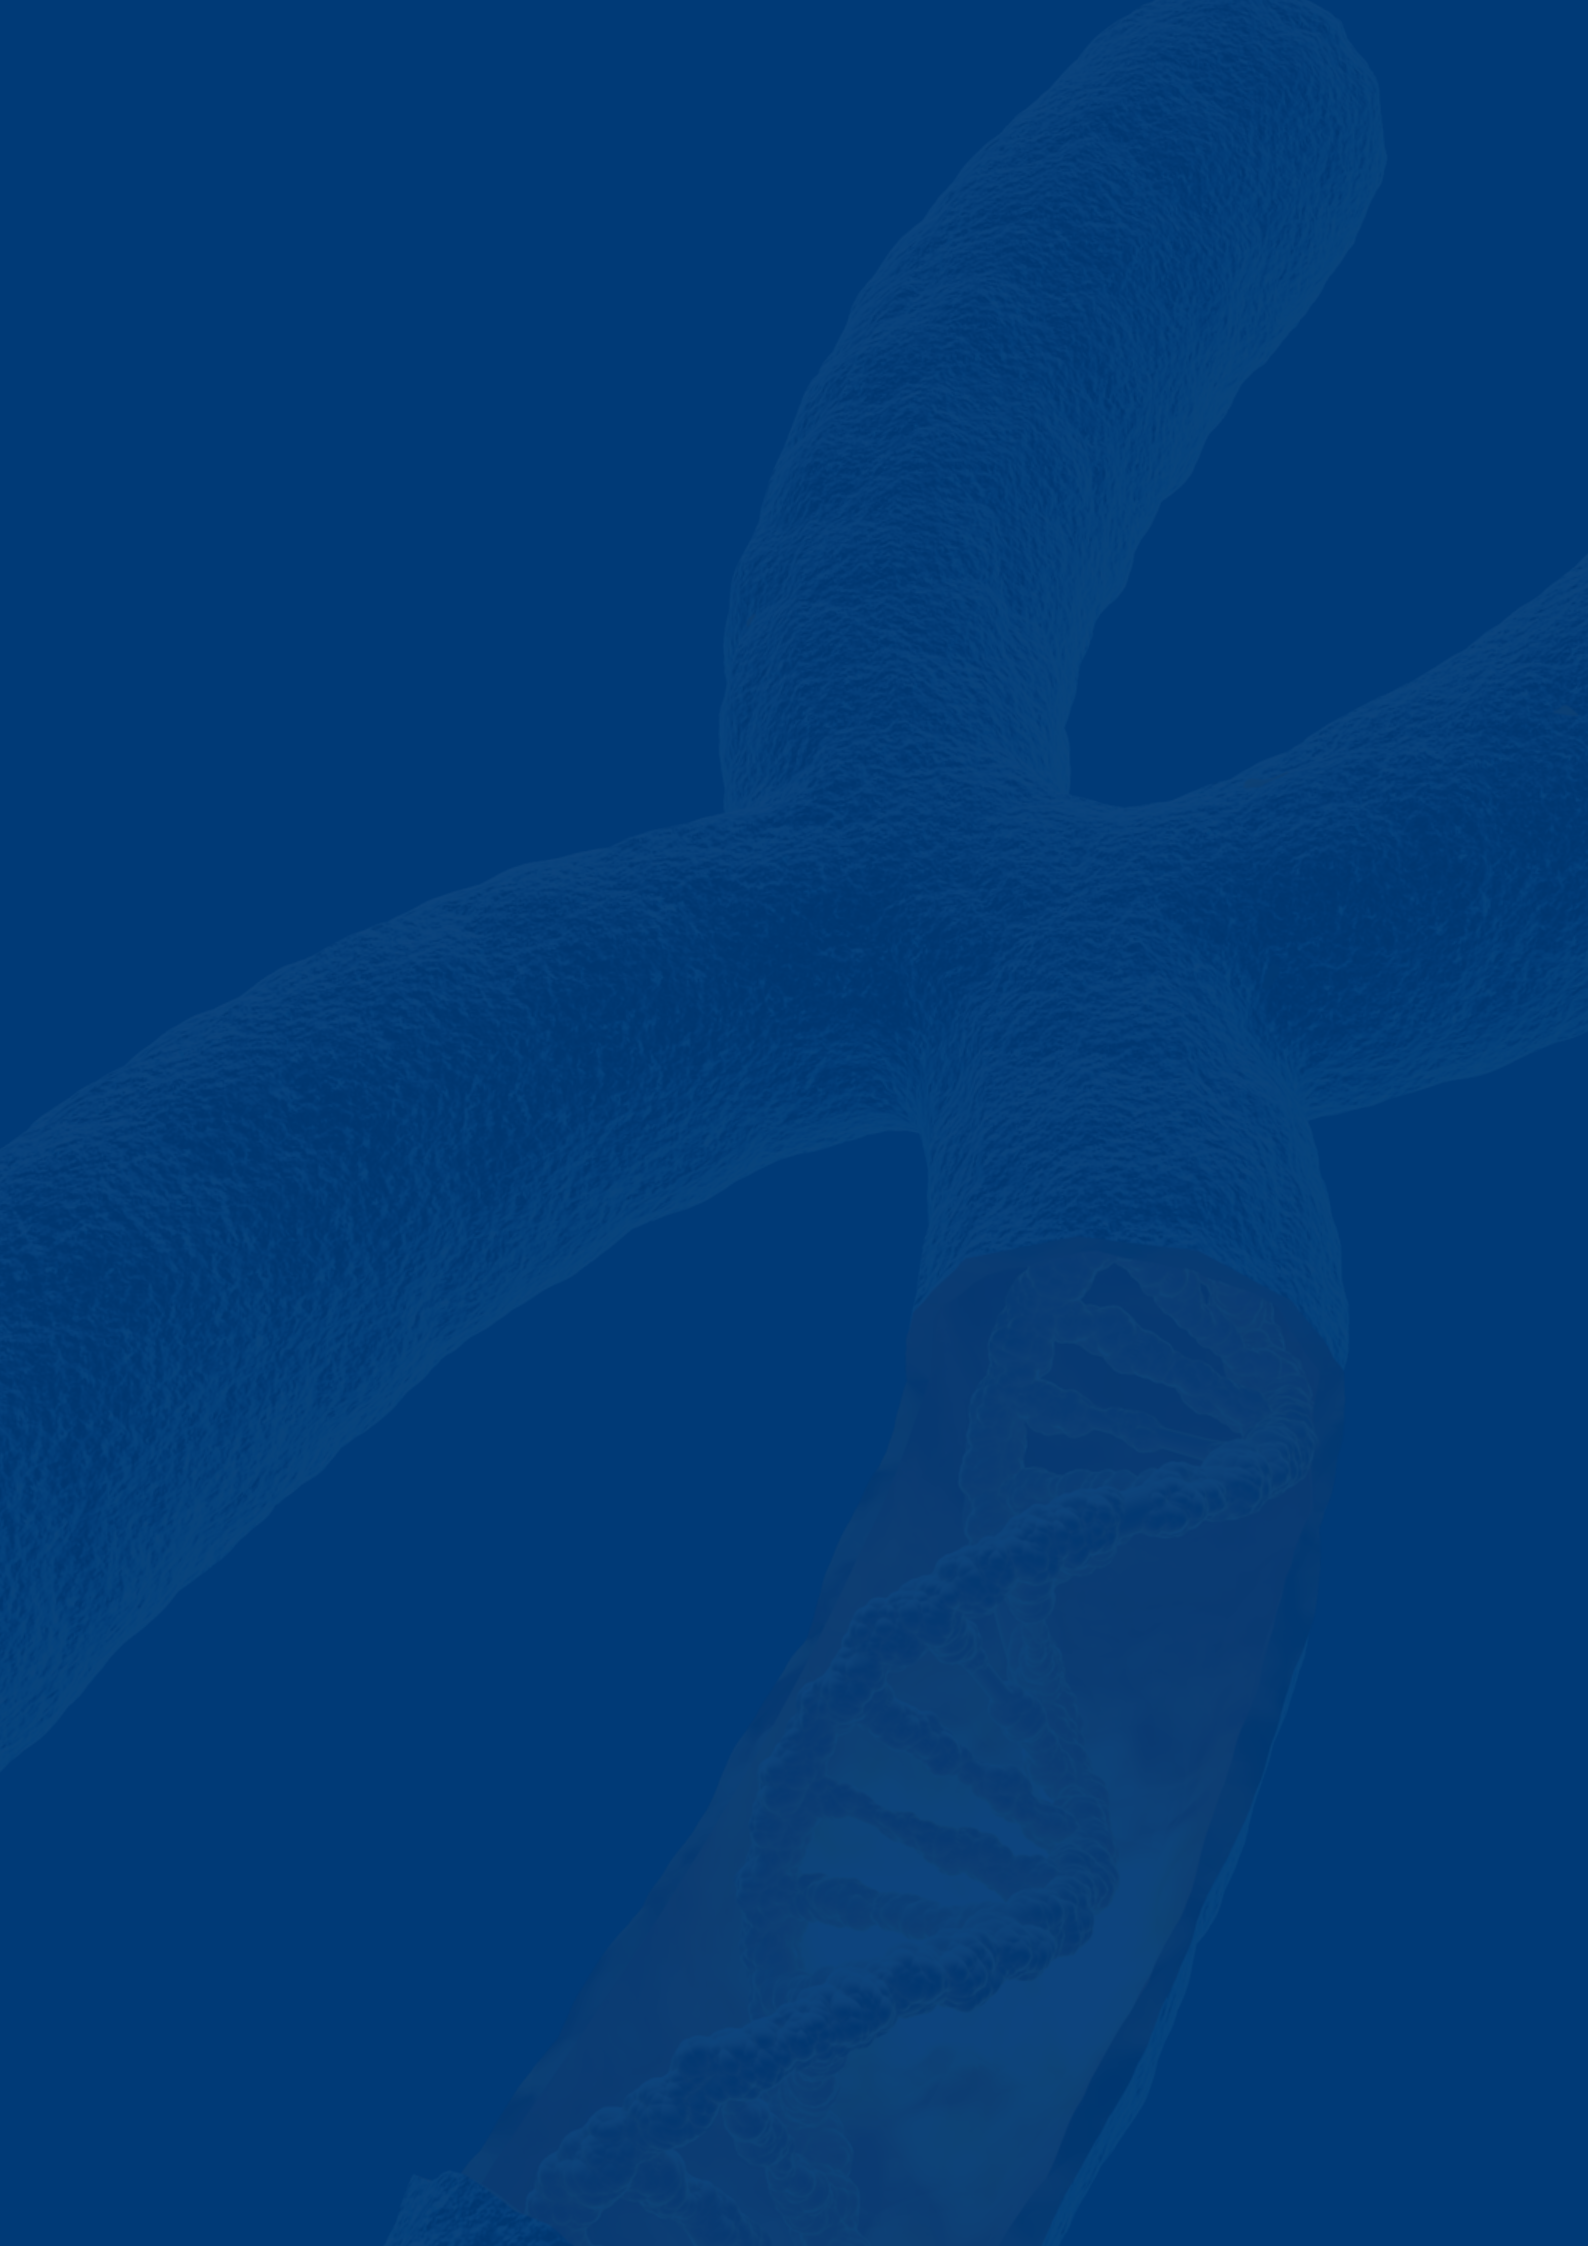

PHARMALINE MOLECULAR BIOLOGY REAGENTS

PharmaLine Healthcare Services Industry and Trade Inc.

PHARMALINE offers solutions that meet global standards in the field of molecular biology, in vitro diagnostics (IVD), and high-purity chemical reagents.
All our products are manufactured in cGMP certified facilities and in accordance with ISO 9001/ISO 13485 guidelines to guarantee the highest purity and consistency, from disease diagnosis to scientific project executions and clinical research.
Our manufacturing philosophy is to ensure the reliability and reproducible results that form the foundation of your laboratory work.

About Us

PharmaLine Healthcare Services Industry and Trade Inc. develops and manufactures molecular diagnostic kits and high-purity laboratory reagents for oncology, microbiology and medical genetics. Our products are designed in our in-house R&D laboratory and manufactured in cGMP-certified facilities under a quality management system aligned with ISO 9001 and ISO 13485.
Our manufacturing approach is built on reliability and reproducibility, so that laboratories can depend on consistent results from run to run.
Our commitments

- cGMP manufacturing: Standardized production on robotic lines, in compliance with international quality standards.
- Responsiveness: A focused, agile organization that supports healthcare professionals with fast, practical solutions.
- Patient benefit: Accessible, reliable diagnostics that help clinicians reach accurate results sooner.







PRODUCT CATALOG

Reagents for Molecular Biology Research

CONTENTS

01 MOLECULAR KITS & IVD PRODUCTS

A. Viral Detection and Genotyping Kits
- UniPatogen CerviPan HPV qPCR Screening Kit (Broad Screening)
- UniPatogen CerviDX12 HPV Genotyping Kit
- UniPatogen CerviDX15 HPV Genotyping Kit (15 High-Risk Types)
- UniPatogen CMV qPCR Quantitative Detection Kit
- MultiPatogen RespiroScan-4 Kit (Multiplex Respiratory Panel)
- CoviScope RT-qPCR Kit (SARS-CoV-2)
- MonkeyPox qPCR Kit (Clade-I & Clade-II Genotyping)

B. Bacterial and Parasitic Kits
- MultiPatogen Gastroenteritis qPCR Panel
- MultiPatogen TriPorter qPCR Kit (MRSA, S. typhi, GAS)
- Malaria Detection Kit (Plasmodium spp.)

C. Genetic Screening Kits
- Xplogen SMA qPCR Screening Kit (SMN1 Exon 7 Deletion)

02 CHEMICAL PRODUCTS

A. Special Solutions

PHARMALINE

ONCOLOGY | MICROBIOLOGY | MEDICAL GENETICS



PHARMALINE

ONCOLOGY | MICROBIOLOGY | MEDICAL GENETICS



01

Molecular Kits & IVD Products

UniPatogen

CE 2962 IVD

CerviPan HPV qPCR Screening Kit **Cat No:PHCPN 50/100/250/500/1000**

Product Overview and Targets

The CerviPan HPV qPCR Screening Kit is an in vitro diagnostic tool designed for the rapid and accurate diagnosis of viral agents in nucleic acid isolates obtained from cervical swab specimens. The kit operates on the principle of real-time PCR (qPCR), targeting specific genomic DNA regions of the pathogen. It is applied to samples from women suspected of having an illness by healthcare providers.

This kit performs a comprehensive screening for high-risk HPV types using **4-channel** qPCR instruments, utilizing a **two-mix structure (Primer Mix 1 and Primer Mix 2)** to cover a broad spectrum of oncogenic risk:

- **Primer Mix 1** utilizes four different channels (FAM, HEX, ROX, CY5) to detect HPV 16, HPV 18, and HPV 45, along with the Internal Control (IC).
- **Primer Mix 2** utilizes the FAM and HEX channels to detect additional high-risk types, including HPV 31, 33, 35, 39, 51, 52, 56, 58, 59, 66, and 68. This mix also includes the Internal Control (IC).
- Internal Control (IC): Both mixes contain the Human RNase P gene to control for specimen quality.

Key Features

- Speed: Diagnosis can be completed in less than 1 hour (validated with Bio-Rad CFX96 Touch).
- Broad Screening: Provides wide coverage for critical high-risk HPV types across two mixes.
- Analytical Performance: Pre-clinical optimization and validation were performed using positive control clones from the Karolinska Institute's International Human Papillomavirus Reference Center, confirming high sensitivity, specificity, and linearity.
- Reliability: Includes Negative Control (NTC) and Positive Control (PC) for contamination and reagent stability control.
- Certification: CE IVD marked and strictly for professional in vitro diagnostic use only.

Technical Details and Storage

- Sample Type: Nucleic acid isolates from cervical swabs.
- Storage Temperature: Must be stored below (-15)°C.
- Shelf Life: 12 months.

UniPatogen

CE 2962 IVD

CerviPan HPV qPCR Screening Kit **Cat No:PHCPN 50/100/250/500/1000**

Validation Data

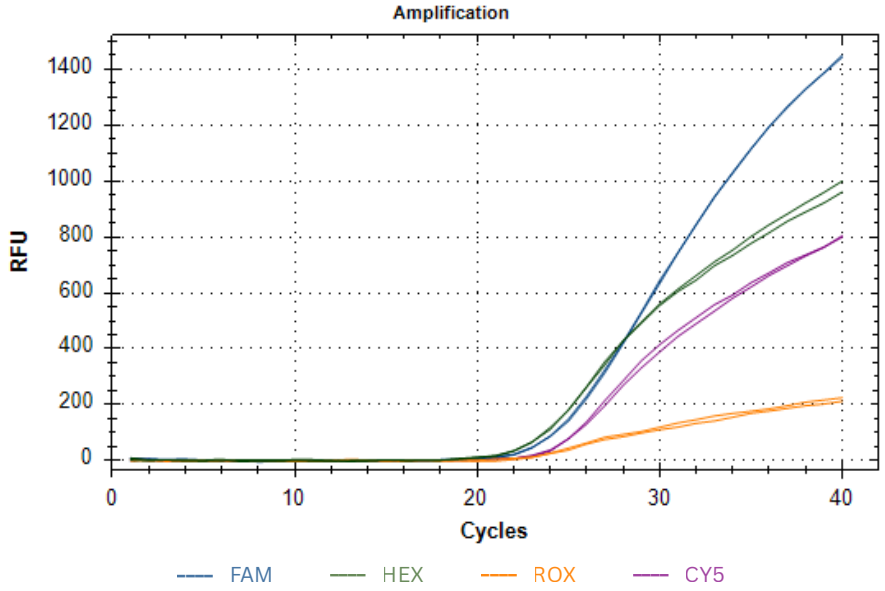


Figure 1. **Primer Mix-1 (Types 16, 18, 45):** Positive results are indicated by FAM (+) for HPV 16, HEX (+) for HPV 18, and ROX (+) for HPV 45. When all target channels are negative, Cy5 (Internal Control) must be positive; otherwise, the test is invalid. If any target channel is positive, the result is considered valid even if the IC is negative.

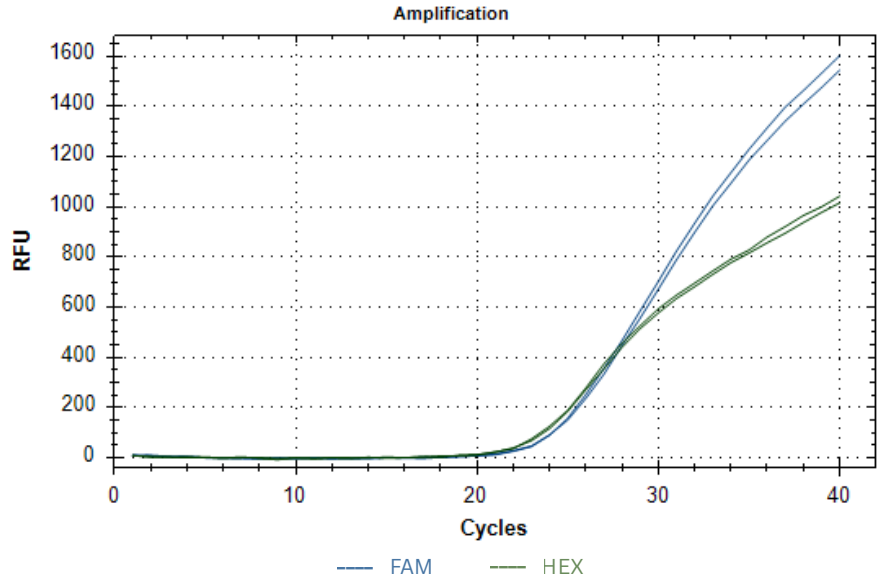


Figure 2. **Primer Mix-2 (Other High-Risk Types)**: A FAM (+) result indicates positivity for at least one of the following HPV types: 31, 33, 35, 39, 51, 52, 56, 58, 59, 66 and 68. When FAM is negative, HEX (Internal Control) must be positive. If both channels are negative, the test is considered invalid.

UniPatogen

CE IVD

UniPatogen CerviDX12 HPV Genotyping Kit **Cat No: PHCDX12 100/250**

Product Overview and Targets

The CerviDX12 HPV Genotyping Kit is developed for the rapid and accurate diagnosis of viral agents in nucleic acid isolates from cervical, penis, and vaginal swabs using real-time PCR (qPCR).

Utilizing **4 distinct primer mixes** across separate reaction tubes, the kit simultaneously detects 12 high-risk HPV types:

- **Primer Mix 1:** Targets HPV 39 (FAM), HPV 52 (HEX), HPV 35 (ROX), and the Human RNase P gene Internal Control (CY5).
- **Primer Mix 2**: Targets HPV 33 (FAM), HPV 6/11 (HEX), HPV 68 (ROX), and the Internal Control (CY5).
- **Primer Mix 3:** Targets HPV 51 (FAM), HPV 56 (HEX), HPV 31 (ROX), and the Internal Control (CY5).
- **Primer Mix 4:** Targets HPV 66 (FAM), HPV 58 (HEX), HPV 59 (ROX), and the Internal Control (CY5).

Key Features

- Speed: Diagnosis can be completed in less than 1 hour using validated instruments like the Bio-Rad CFX96 Touch.
- Multiplex Genotyping: Offers simultaneous detection and genotyping of 12 distinct HPV types, essential for clinical risk assessment.
- Analytical Performance: Pre-clinical optimization and validation were performed using positive control clones from the Karolinska Institute's International Human Papillomavirus Reference center, ensuring high specificity and reliability.
- Reliability: Includes Negative Control (NTC) and Positive Control (PC) for contamination and reagent stability control in every run.
- Certification: CE IVD marked and strictly for professional in vitro diagnostic use only.

Technical Details and Storage

- Kit Components: The kit consists of a 2X Master Mix (containing DNA polymerase, dNTP mix, reaction buffer) and four distinct Primer Mixes.
- Storage Temperature: Must be stored below (-15)°C.
- Shelf Life: 12 months.

UniPatogen

CE IVD

UniPatogen CerviDX12 HPV Genotyping Kit **Cat No: PHCDX12 100/250**

Validation Data

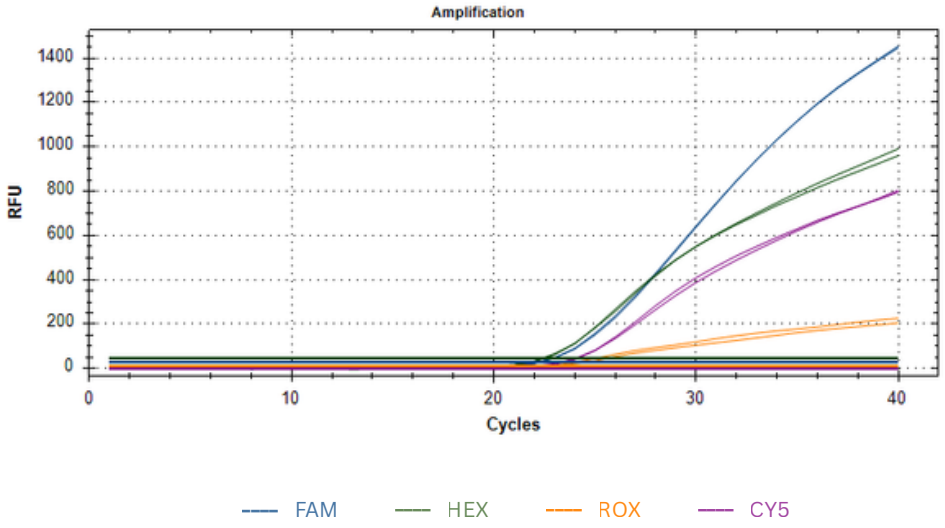


Figure 1. **Positive Amplification Profile:** The plot demonstrates specific signal accumulation exceeding the threshold in at least one of the target channels (FAM: 39, 33, 51, 66; HEX: 52, 6/11, 56, 58; ROX: 35, 68, 31, 59). Detected positivity in the target channels is considered diagnostically valid, independent of the CY5 (RNase P) internal control signal.

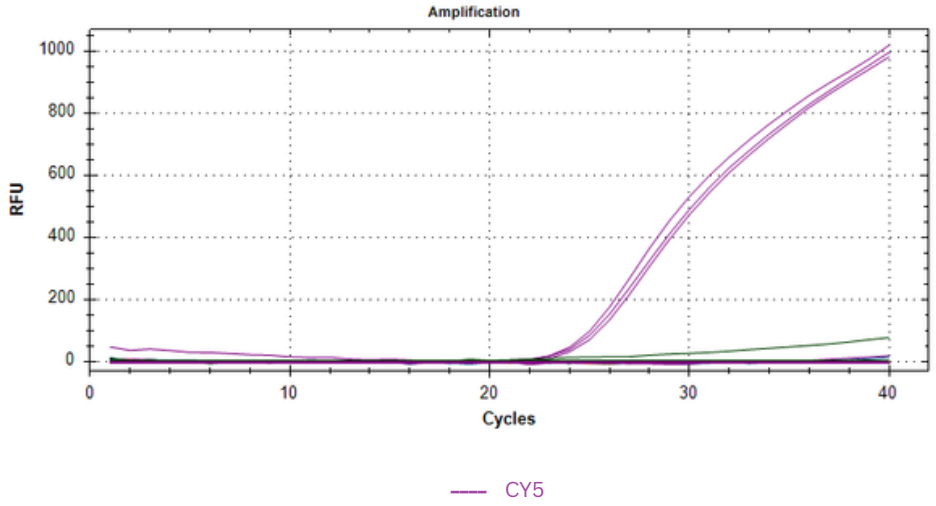


Figure 2. **Negative Amplification Profile:** No signal increase was detected in the target channels (FAM, HEX, ROX). The extraction quality and PCR performance are confirmed by the positive signal in the CY5 (RNase P) internal control channel. Instances where all channels are negative are considered invalid, and the test must be repeated.

UniPatogen

CE IVD

UniPatogen CerviDX15 HPV Genotyping Kit **Cat No: PHCDX15 100/250**

Product Overview and Targets

The CerviDX15 HPV Genotyping Kit is an in vitro diagnostic tool designed for the rapid and accurate diagnosis of viral agents in nucleic acid isolates from cervical, penis, and vaginal swab specimens using real-time PCR (qPCR). Utilizing **5 distinct primer mixes** across separate reaction tubes, the kit simultaneously detects and genotypes 15 high-risk HPV types:

- **Primer Mix 1:** Targets HPV 39 (FAM), HPV 52 (HEX), HPV 35 (ROX), and the Human RNase P gene Internal Control (CY5).
- **Primer Mix 2:** Targets HPV 33/6/11 (FAM/HEX), HPV 68 (ROX), and the Internal Control (CY5).
- **Primer Mix 3:** Targets HPV 51 (FAM), HPV 56 (HEX), HPV 31 (ROX), and the Internal Control (CY5).
- **Primer Mix 4:** Targets HPV 66 (FAM), HPV 58 (HEX), HPV 59 (ROX), and the Internal Control (CY5).
- **Primer Mix 5:** Targets HPV 16 (FAM), HPV 18 (HEX), HPV 45 (ROX), and the Internal Control (CY5).

Key Features

- Speed: Diagnosis can be completed in less than 1 hour (validated with Bio-Rad CFX96 Touch).
- Comprehensive Genotyping: Offers simultaneous detection and genotyping of 15 distinct high-risk HPV types.
- Analytical Performance: Pre-clinical optimization and validation were performed using positive control clones from the Karolinska Institute's International Human Papillomavirus Reference center , confirming high sensitivity, specificity, and linearity.
- Reliability: Includes Negative Control (NTC) and Positive Control (PC) for contamination and reagent stability control.
- Certification: CE IVD marked and strictly for professional in vitro diagnostic use only.

Technical Details and Storage

- Sample Type: Nucleic acid isolates from cervical, penis, and vaginal swabs.
- Storage Temperature: Must be stored below (-15)°C.
- Shelf Life: 12 months.

UniPatogen

CE IVD

UniPatogen CerviDX15 HPV Genotyping Kit **Cat No: PHCDX15 100/250**

Validation Data


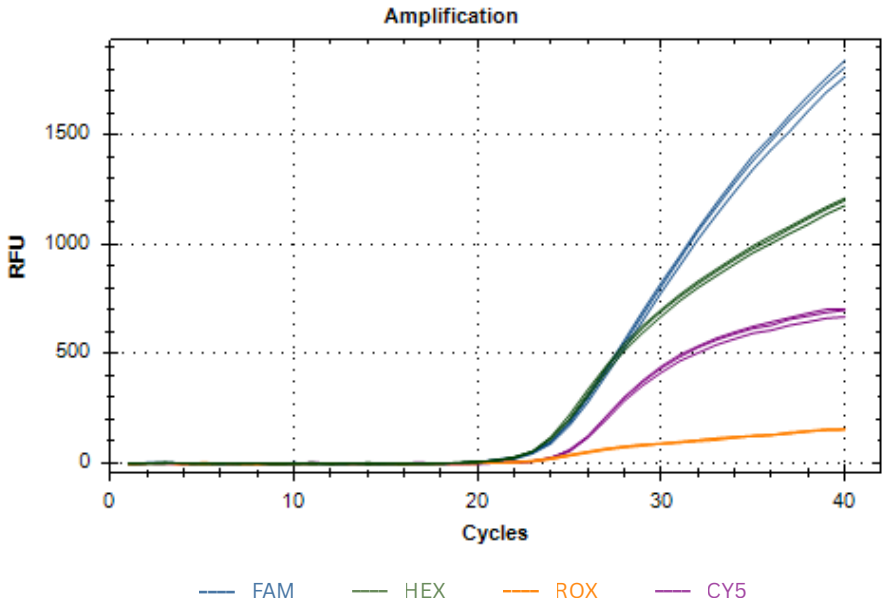


Figure 1. **Positive Amplification Profile:** The plot demonstrates specific signal accumulation exceeding the threshold in at least one of the target channels (FAM: 39, 33, 51, 66, 16; HEX: 52, 6/11, 56, 58, 18; ROX: 35, 68, 31, 59, 45). Detected positivity in the target channels is considered diagnostically valid, independent of the CY5 (RNase P) internal control signal.

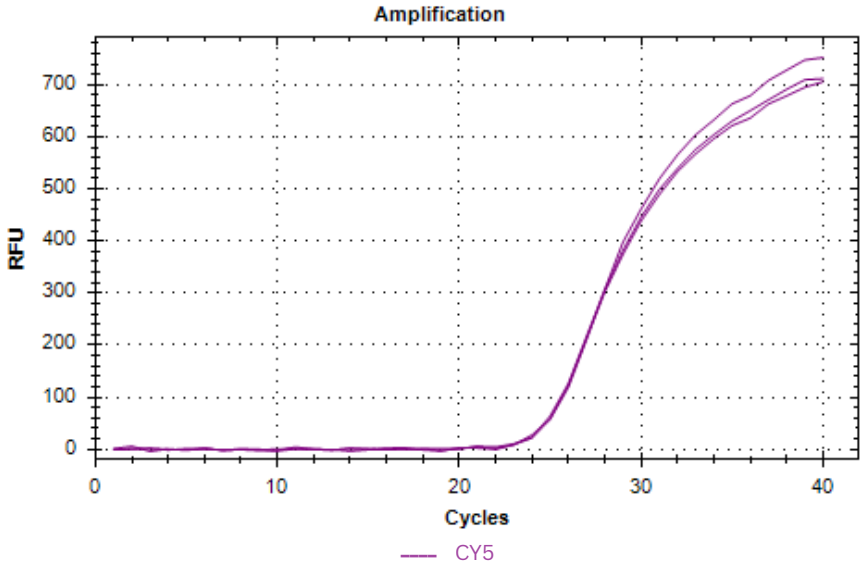

F*igure 2.* **Negative Amplification Profile:** No signal increase was detected in the target channels (FAM, HEX, ROX). The extraction quality and PCR performance are confirmed by the positive signal in the CY5 (RNase P) internal control channel. Instances where all channels are negative are considered invalid, and the test must be repeated.

UniPatogen

RUO

UniPatogen CMV qPCR Quantitative Detection Kit **Cat No: PHCMV 500/100**

Product Overview and Objectives

The UniPatogen CMV qPCR Quantitative Detection Kit is an in vitro diagnostic (IVD) tool designed for the rapid, accurate, and quantitative (viral load) determination of Cytomegalovirus (CMV) presence in clinical samples. The kit is applied to nucleic acid isolates obtained from various sample types, such as human blood, plasma, serum, urine, stool, bronchoalveolar lavage (BAL), cerebrospinal fluid (CSF), amniotic fluid, and ocular fluid.

Diagnosis and viral load monitoring are performed using the Real-Time PCR (qPCR) method targeting a conserved region of the CMV genome, alongside a standard curve generated using standards of known concentrations. The panel utilizes two primary channels:

- FAM Channel: CMV Target Region.
- CY5 Channel: *Internal Control (Human beta-actin gene).*

Key Features

- Speed: The diagnostic and quantification process is completed in approximately 1 hour and 26 minutes using validated instruments such as the Bio-Rad CFX96 Touch.
- Broad Sample Matrix: Demonstrates high performance in isolates obtained from blood, plasma, serum, urine, stool, BAL, CSF, amniotic, and ocular fluids.
- Precise Quantification: Provides precise viral load determination within a wide linear range ($R^2 \geq 0.98$).
- Reliability: Includes an Internal Control (IC) to verify isolation and amplification efficiency, as well as Positive (PC) and Negative (NTC) controls to monitor reagent stability and contamination.

Storage Conditions

- Kit Components: Contains 2X Master Mix, Target Primer Mix (CMV FAM + IC CY5), and Control Reagents (PC, NTC).
- Storage Temperature: Must be stored below -15°C. After initial thawing, components can be stored short-term at 2°C to 8°C ; repeated freeze-thaw cycles should be avoided.
- Shelf Life: 12 months.
- Validated Instruments: Validated for use with Bio-Rad CFX96 Touch, Qiagen Rotor-Gene Q, and Thermo Fisher QuantStudio systems.

UniPatogen

RUO

UniPatogen CMV qPCR Quantitative Detection Kit **Cat No: PHCMV 500/100**

Doğrulama Verileri

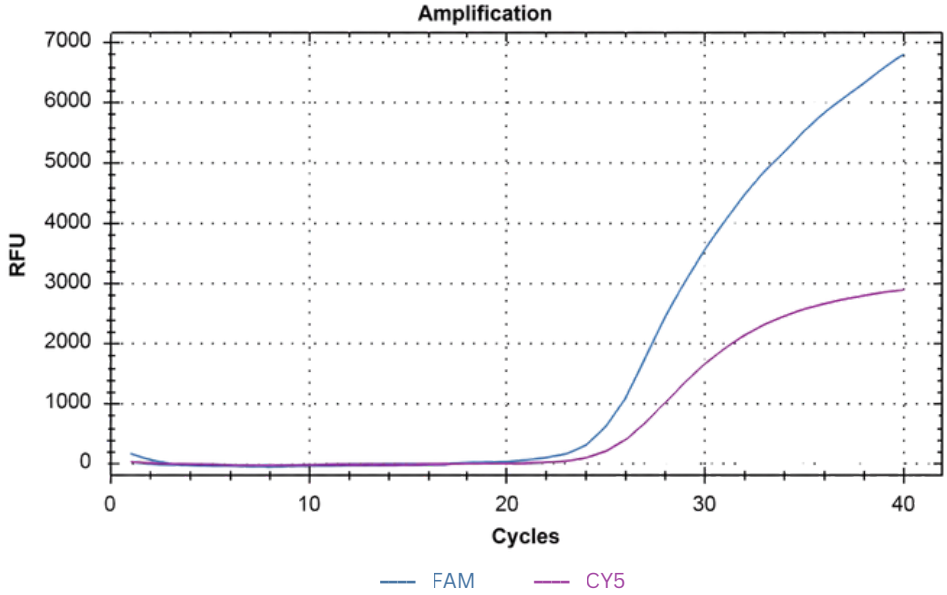


Figure 1. **Positive Amplification Profile:** The graph demonstrates the specific signal increase exceeding the threshold in the CMV target channel (FAM). Positivity detected in the FAM channel is considered valid for viral load quantification. Meanwhile, the positivity of the internal control signal (CY5 - Human Beta-actin) confirms the success of the reaction.

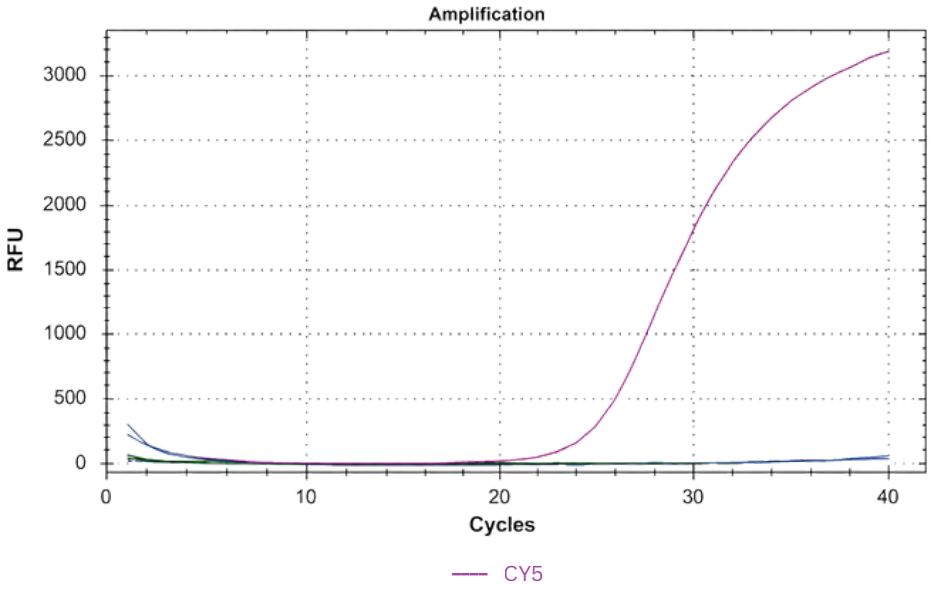


Figure 2. **Negative Amplification Profile:** No signal increase was detected in the CMV target channel (FAM) (no CMV DNA detected). Extraction quality and PCR reaction success are confirmed by the positivity of the internal control signal (Human Beta-actin) in the CY5 channel. Cases where both the FAM and CY5 channels are negative are considered invalid, and the test must be repeated.

MultiPatogen

RUO

MultiPatogen RespiroScan-4 RT-qPCR Kit **Cat No: PHMP4 1000**

Product Overview and Targets

The MultiPatogen RespiroScan-4 Kit is developed for the rapid and accurate diagnosis of viral agents in nucleic acid isolates obtained from clinical specimens (e.g., nasopharyngeal swabs, sputum). The kit operates via single-step RT-qPCR, targeting specific genomic RNA regions.

It simultaneously detects critical respiratory pathogens using **4-channel** instruments:

- SARS COV-2 ORF1ab (FAM)
- Influenza A&B (HEX)
- Respiratory Syncytial Virus (RSV) A/B (ROX)
- Internal Control (IC): Human RNaseP gene (CY5) for controlling specimen quality and inhibition.

Key Features

- Speed: Diagnosis can be completed in less than 1 hour (validated with Bio-Rad CFX96 Touch).
- Sensitivity: Provides excellent analytical performance, determined using synthetic pUC57 plasmid.
- Reliability: Includes Negative Control (NTC) and Positive Control (PC) for contamination and reagent stability control in every run.
- Certification: CE IVD marked and strictly for professional in vitro diagnostic use.

Storage

- Storage Temperature: Stable between (-15°C) and (-25°C)
- Shelf Life: 12 months.

MultiPatogen

RUO

MultiPatogen RespiroScan-4 RT-qPCR Kit **Cat No: PHMP4 1000**

Validation Data

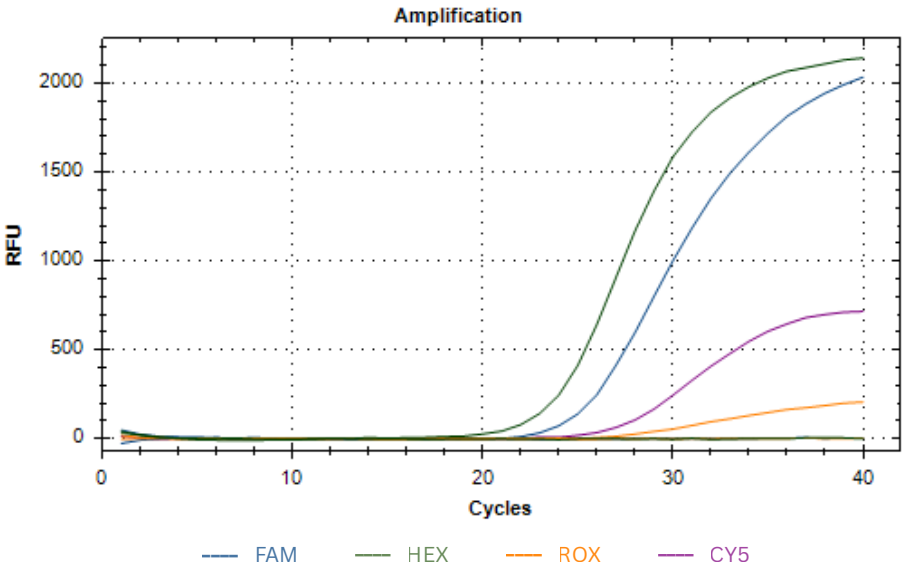


Figure 1. **Positive Amplification Profile**: The plot demonstrates specific signal accumulation exceeding the threshold in at least one of the target channels: FAM (SARS-CoV-2 ORF1ab), HEX (Influenza A&B), or ROX (RSV A/B). Detected positivity in target channels is diagnostically valid, regardless of the CY5 (Internal Control - RNase P) signal.

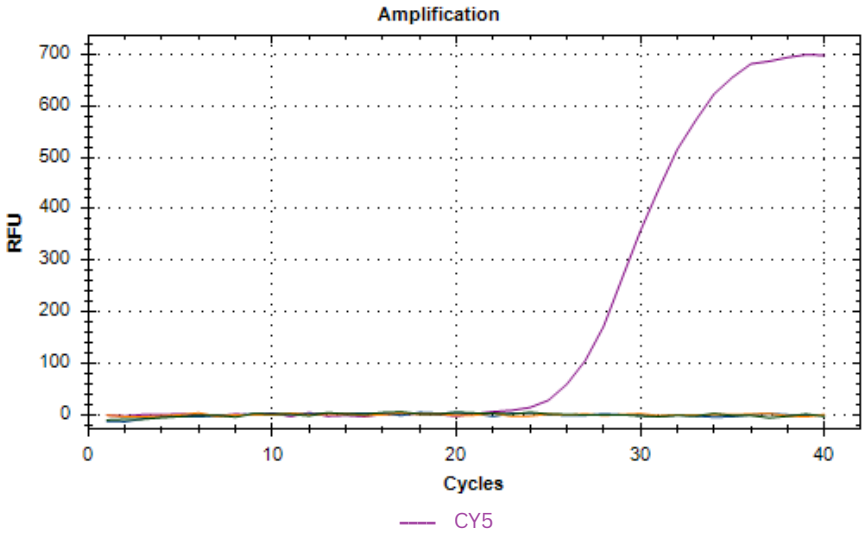


Figure 2. **Negative Amplification Profile:** No specific amplification was detected across the FAM, HEX, or ROX target channels. Analytical validity and sample integrity are confirmed by the positive signal in the CY5 (Internal Control - RNase P) channel. If all channels remain negative, the test is considered invalid and must be repeated.

UniPatogen

RUO

UniPatogen CoviScope RT-qPCR Kit **Cat No: PHMCVSP 100/1000**

Product Overview and Targets

The Unipatogen CoviScope RT-qPCR Kit is an in vitro diagnostic tool designed for the qualitative detection of the genomic RNA of the SARS-CoV-2 coronavirus, the causative agent of COVID-19. It utilizes a specific Taqman probe system.

The kit is applied to nucleic acid isolates obtained from clinical specimens, including nasopharyngeal swabs, oropharyngeal swabs, bronchoalveolar lavage, nasopharyngeal aspirates, and sputum. The diagnosis is performed using a single-step Reverse Transcription (RT) and real-time PCR (qPCR) method (RT-qPCR) targeting specific genomic RNA regions.

This solution simultaneously targets the following genes using 2-channel qPCR instruments:

- SARS COV-2 (ORF1ab & N genes) (FAM)
- Internal Control (IC): Human RNaseP gene (HEX) for controlling specimen quality and potential qPCR inhibition.

Key Features

- Speed: Diagnosis can be completed in less than 1 hour (validated with Bio-Rad CFX96 Touch).
- Dual Target Detection: Targets two key regions of the SARS-CoV-2 genome (ORF1ab & N) for robust confirmation.
- Analytical Performance: Performance studies were carried out using synthetic SARS-CoV-2 RNA fragments, demonstrating high analytical quality ($R^2 = 0.9909$).
- Reliability: Includes Negative Control (NTC) and Positive Control (PC) for contamination and reagent stability control in every run.
- Certification: CE IVD marked and strictly for professional in vitro diagnostic use only.

Technical Details and Storage

- Sample Type: Includes 2X Master Mix (containing DNA polymerase, reverse transcriptase, dNTP mix, and inhibitor) and a Primer Mix.
- Storage Temperature: Stable between (-15°C) and (-25°C)
- Shelf Life: 12 months.

UniPatogen

RUO

UniPatogen CoviScope RT-qPCR Kit **Cat No: PHMCVSP 100/1000**

Validation Data

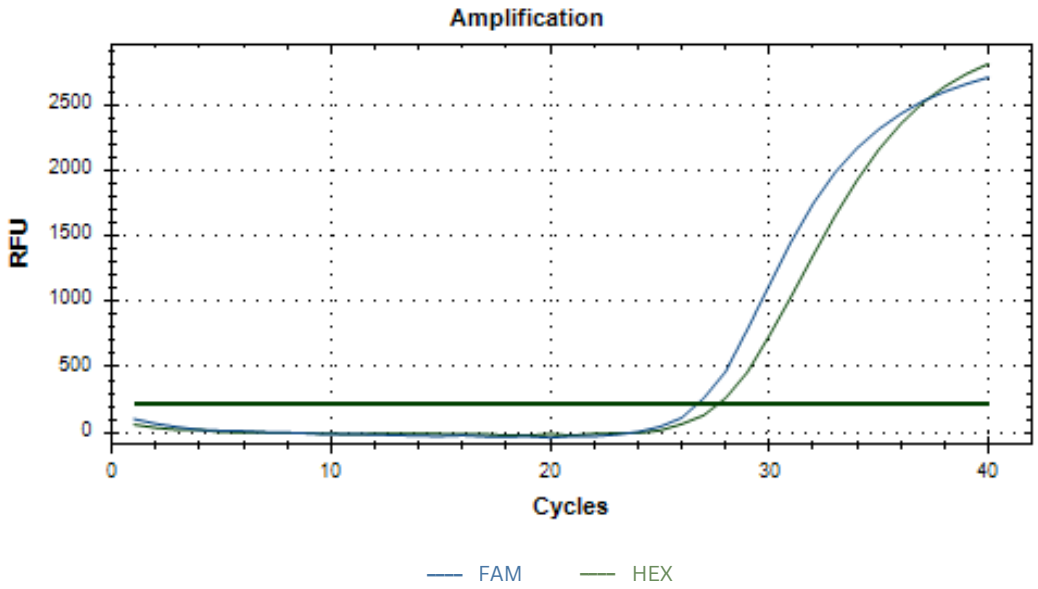


Figure 1. **Positive Amplification Profile:** The plot demonstrates a specific signal increase exceeding the threshold in the target channel (FAM: SARS-CoV-2 ORF1ab and N genes). Positivity detected in the target channel is diagnostically valid, regardless of the HEX (Internal Control - RNase P) signal.

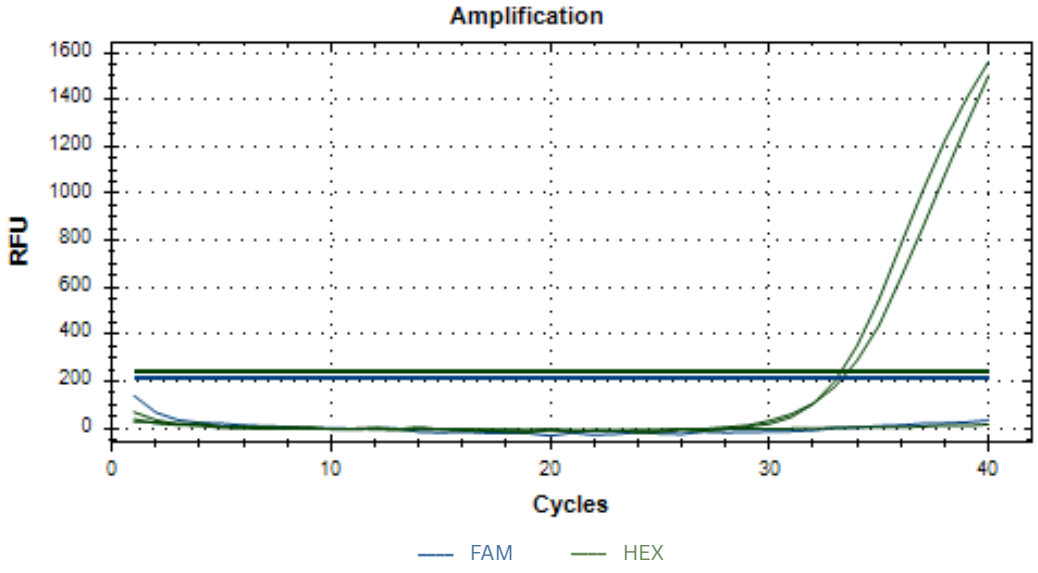


Figure 2. **Negative Amplification Profile:** No specific signal increase was detected in the target channel (FAM). Analytical validity and sample integrity are confirmed by the positive signal in the HEX (Internal Control - RNase P) channel. If both channels are negative, the test is considered invalid and must be repeated.

PHARMALINE®

RUO

MonkeyPox qPCR Kit **Cat No: PHMNKY2022 100/500**

Product Overview and Targets

The Pharmaline MonkeyPox qPCR Kit is developed for the rapid and accurate diagnosis of viral agents in nucleic acid isolates obtained from clinical specimens, specifically using swab samples collected from skin lesions. Diagnosis is performed using real-time PCR (qPCR), targeting specific genomic DNA regions of the pathogen.

This solution enables the qualitative detection and genotyping of the MonkeyPox virus.

Detected Targets and Key Advantages

The kit utilizes 4-channel qPCR instruments and specific probes to detect and differentiate the two major MonkeyPox clades:

- Detects the MonkeyPox Generic (G2R) gene, providing general confirmation of the virus's presence. (FAM)
- Detects MonkeyPox Type-2 (Clade-II) (F3L), allowing for the differentiation of the West African Clade. (HEX)
- Detects MonkeyPox Type-1 (Clade-I) (F3L), allowing for the differentiation of the Central African Clade. (ROX)
- Detects the Internal Control (IC) (Human RNaseP gene), which controls for sample quality and PCR inhibition (CY5)

Key Features

- Genotyping Capability: Allows differentiation (genotyping) between the more severe Central African Clade-I and the West African Clade-II.
- Speed: Diagnosis can be completed in less than 1 hour (validated with Bio-Rad CFX96 Touch).
- Reliability: Includes Negative Control (NTC) and Positive Control (PC) for contamination and reagent stability control.
- Certification: CE IVD marked and strictly for professional in vitro diagnostic use only.

Technical Details and Storage

- Sample Type: Nucleic acid isolates from skin lesion swabs.
- Storage Temperature: Stable between (-15°C) and (-25°C)
- Shelf Life: 12 months.

PHARMALINE®

RUO

MonkeyPox qPCR Kit **Cat No: PHMNKY2022 100/500**

Validation Data

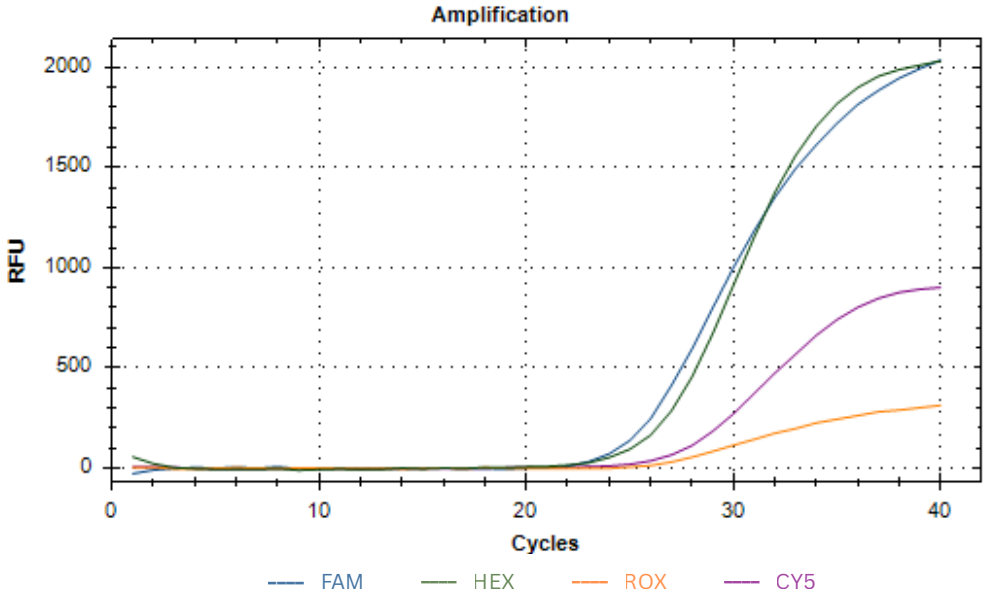


Figure 1. **Positive Amplification Profile:** The plot demonstrates specific fluorescence accumulation exceeding the threshold in at least one of the target channels: FAM (Mpox Generic - G2R), HEX (Clade-II / West African), or ROX (Clade-I / Central African). Detected positivity in target channels is diagnostically valid, regardless of the CY5 (Internal Control - RNase P) signal. Simultaneous detection in generic and clade-specific channels provides a definitive confirmation of virus presence and clade differentiation.

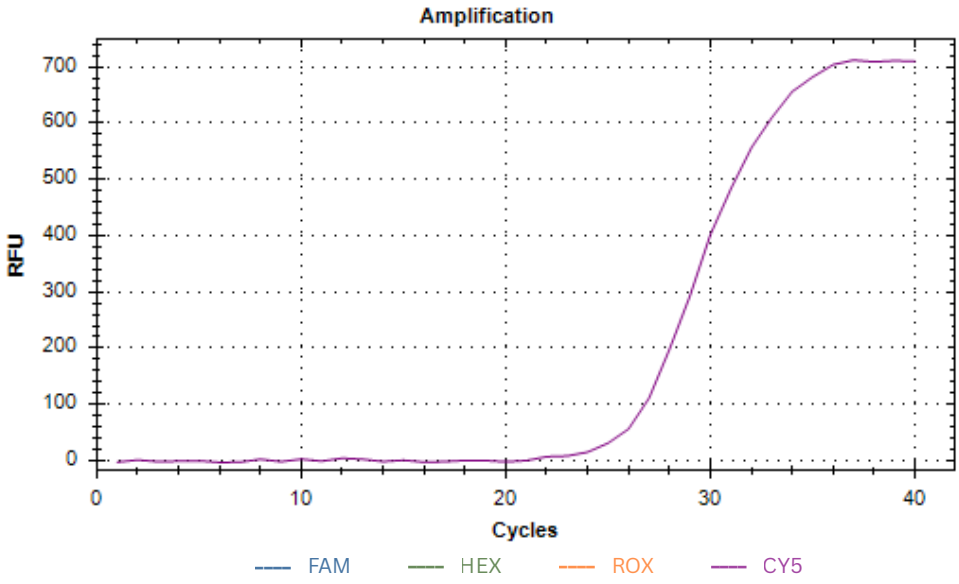


Figure 2. **Negative Amplification Profile:** No specific amplification was detected across the FAM, HEX, or ROX target channels. Analytical validity and sample integrity are confirmed by the positive signal in the CY5 (Internal Control - RNase P) channel. If all channels remain negative, the test is considered invalid and must be repeated.

MultiPatogen

RUO

MultiPatogen Gastroenteritis qPCR Panel **Cat No: PHMPGIS2023 25/50/100**

Product Overview and Targets

The MultiPatogen GIS Gastroenteritis qPCR Panel is an in vitro diagnostic tool designed for the rapid and accurate detection of viral, bacterial, and parasitic agents causing gastrointestinal infections in nucleic acid isolates from rectal swabs and stool samples.

Using one-step RT-qPCR, the panel targets specific genomic regions across **8 specialized primer mixes**:

- **Virüs Primer Mix 1 & 2:** Targets *Astrovirus, Rotavirus, Adenovirus, Norovirus* GI/GII, and *Sapovirus.*
- **Parazit Primer Mix:** Targets *Entamoeba histolytica*, *Cryptosporidium* sp., *Cyclospora cayetanensis*, and *Giardia lamblia.*
- **Bakteri Primer Mix 1–4:** Targets *Salmonella* spp., *Campylobacter* spp., *Yersinia enterocolitica*, *Vibrio species* (cholerae, parahaemolyticus, vulnificus), *Plesiomonas shigelloides*, *Clostridium difficile* (Toxin A/B), *Shigella*/EIEC, EAEC, and STEC (stx1/stx2).
- **Bakteri Primer Mix 5:** Targets EPEC, ETEC, alongside Human Actin and RNaseP Internal Controls (IC).

Key Features

- Speed: Diagnosis can be completed in less than 1 hour using validated devices such as the Bio-Rad CFX96 Touch.
- Comprehensive Panel: Provides extensive screening for viral, bacterial, and parasitic gastroenteritis agents within a single kit.
- Flexibility: Optimized for both RT-qPCR and direct qPCR protocols depending on the target type.
- Reliability: Includes Negative Control (NTC) and Positive Control (PC) in every run to monitor contamination and reagent stability.

Storage


- Kit Components: Contains 2X Taq Mix, 2X RT Mix, target-specific Primer Mixes, and Control Reagents (PC, NTC).
- Storage Temperature: Stable between (-15°C) and (-25°C).
- Shelf Life: 12 months.
- Validated Devices: Validated for use with Bio-Rad CFX96, Qiagen Rotor-Gene Q, and Thermo Fisher QuantStudio systems.

MultiPatogen

RUO

MultiPatogen Gastroenteritis qPCR Panel **Cat No: PHMPGIS2023 25/50/100**

Validation Data

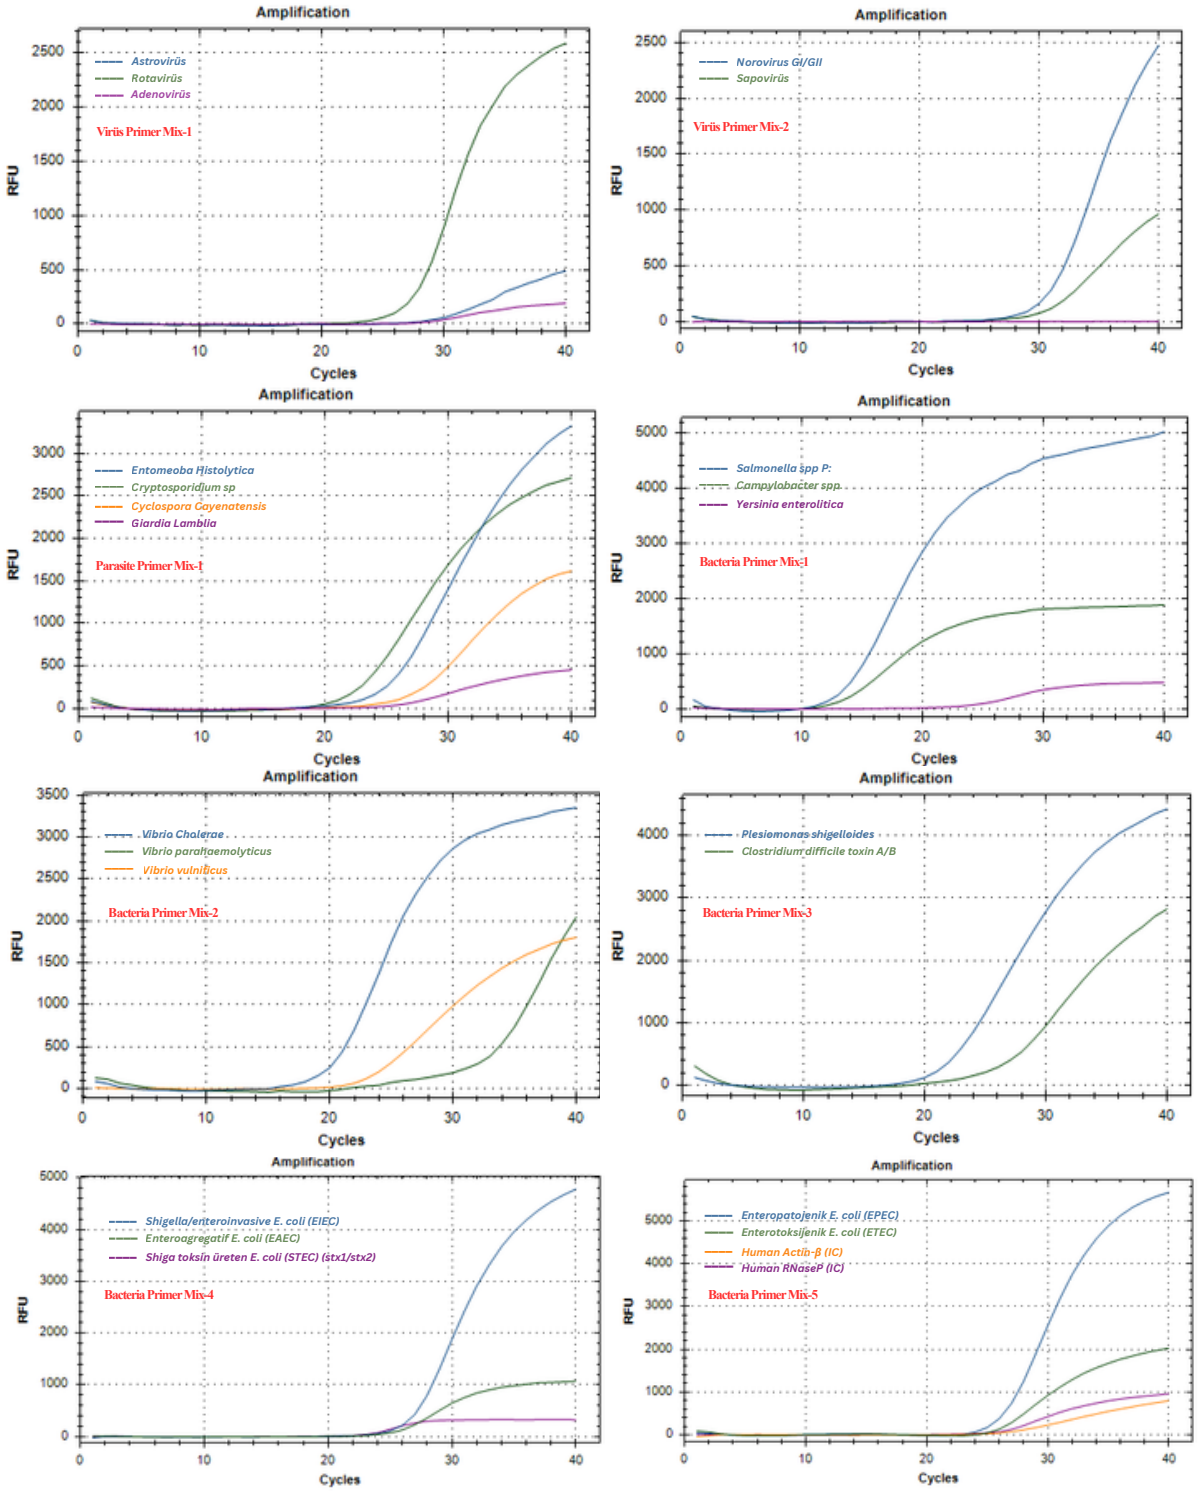

MultiPatogen

RUO

MultiPatogen TriPorter qPCR Kit **Cat No: PHMPPRT2024 50/100/250**

Product Overview and Targets

The MultiPatogen TriPorter qPCR Kit is an in vitro diagnostic tool designed for the rapid and accurate diagnosis of bacterial agents. The kit is applied to nucleic acid isolates obtained from nasopharyngeal swabs and stool samples.

Diagnosis is performed using real-time PCR (qPCR), targeting specific genomic DNA regions of the pathogen

This solution simultaneously detects critical bacterial pathogens using 4-channel qPCR instruments, utilizing all four channels for comprehensive analysis:

- Methicillin-Resistant *Staphylococcus aureus* (MRSA) (FAM)
- *Salmonella typhi* (SAL) (HEX)
- Grup A *Streptococcus* (GAS) (ROX)
- Internal Control (IC): Human RNaseP (CY5)

Key Features

- Speed: Diagnosis can be completed in less than 1 hour (validated with Bio-Rad CFX96 Touch).
- Multiplex Detection: Simultaneous detection of three critical bacterial pathogens (MRSA, *Salmonella typhi,* GAS) in a single run.
- Sample Versatility: Validated for use with both respiratory (nasopharyngeal swab) and gastrointestinal (stool) samples.
- Reliability: Includes Negative Control (NTC) and Positive Control (PC) for contamination and reagent stability control in every run.

Storage

- Kit Components: Includes 2X Master Mix and Primer Mix (containing probes for MRSA, SAL, GAS, and IC).
- Storage Temperature: Stable between (-15°C) and (-25°C).
- Shelf Life: 12 months.
- Stool Sample Preparation: Requires the use of PharmaSEP buffer (PHSP2024-50/100) for proper sample extraction.

MultiPatogen

RUO

MultiPatogen TriPorter qPCR Kit **Cat No: PHMPPRT2024 50/100/250**

Validation Data

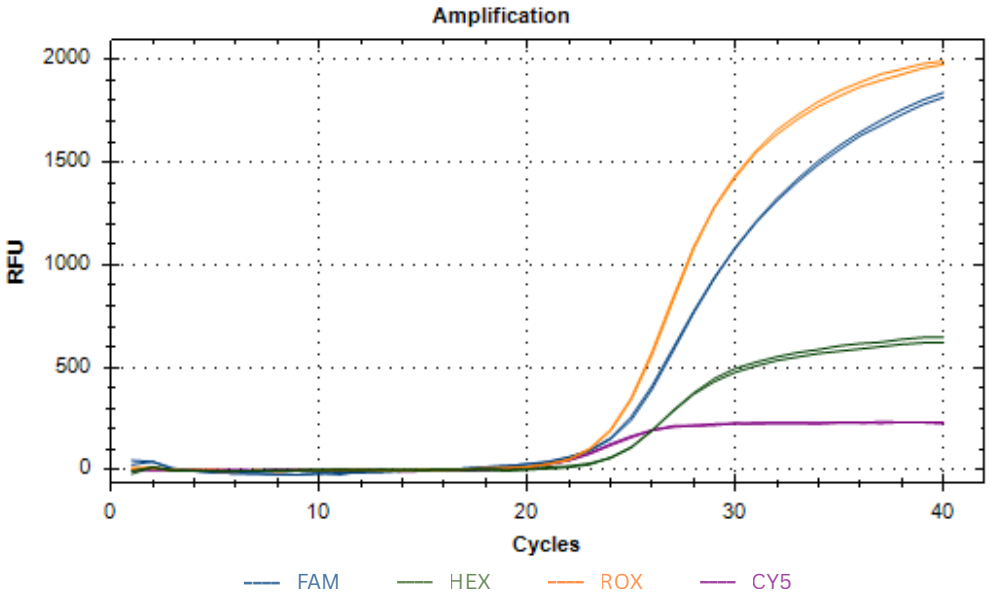


Figure 1. **Positive Amplification Profile:** The plot demonstrates specific fluorescence accumulation exceeding the threshold in at least one of the target channels: FAM (MRSA), HEX (Salmonella typhi), or ROX (GAS). Detected positivity in target channels is diagnostically valid, regardless of the CY5 (Internal Control - RNase P) signal.

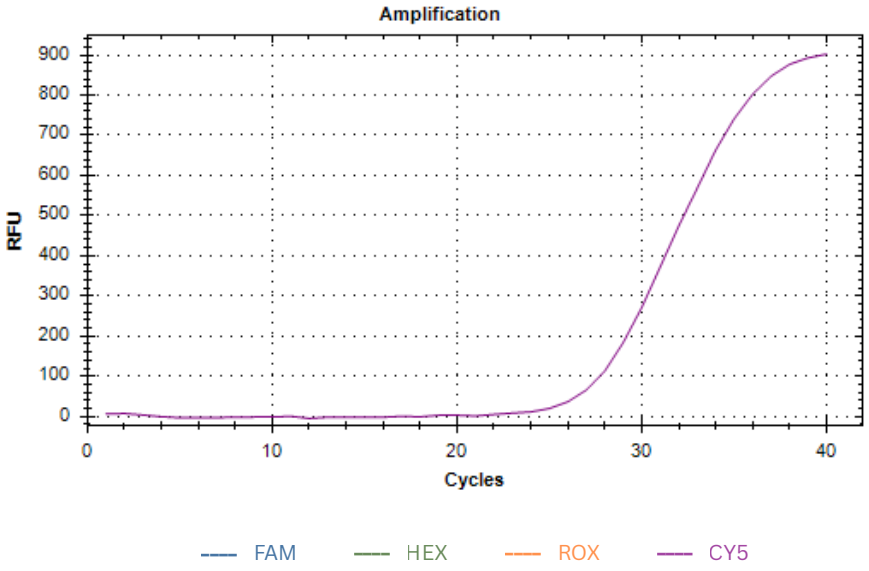


Figure 2. **Negative Amplification Profile:** No specific signal increase was detected in the FAM, HEX, or ROX target channels. Analytical validity and sample integrity are confirmed by the positive signal in the CY5 (Internal Control - RNase P) channel. If all channels remain negative, the test is considered invalid and must be repeated.

PHARMALINE®

RUO

Malaria Detection Kit **Cat No: PHMLR2022 100**

Product Overview and Targets

The Malaria Detection Kit is an in vitro diagnostic tool designed for the highly sensitive and specific detection of all five *Plasmodium* parasite species known to cause malaria. The kit works with Total DNA/Genomic DNA isolated from suspected blood.

Diagnosis is performed using Real-Time PCR (qPCR). The assay is based on a conserved region specific to the 18S rRNA genes of the five *Plasmodium* parasites, using a universal primer-probe design.

The Malaria Detection Kit performs its analysis using two primary fluorescent channels:

- FAM Channel: Used for the detection of *Plasmodium* spp. (all five species of malaria parasite).
- HEX Channel: Used for the Internal Control.

Key Features

- Broad Detection: Capable of detecting all five types of malaria parasites: *Plasmodium vivax, Plasmodium malaria, Plasmodium ovale, Plasmodium falciparum,* and *Plasmodium knowlesi*.
- High Sensitivity: qPCR analysis provides high sensitivity for detecting the parasite's genetic material.
- Compatibility: Fully compatible with Pharmaline Genomic DNA isolation kit (REF: PHDNA2021-100).
- Validated Instruments: Compatible with Biorad® CFX96, LightCycler480 (Roche), and RotorgeneQ (QiaGen).
- Certification: CE IVD marked and strictly for professional use.

Technical Details and Storage

- Sample Type: Total DNA/Genomic DNA isolated from whole blood.
- Shelf Life: 12 months.
- Storage Temperature: Stable between (-15°C) and (-25°C). PCR reagents are stored at -20°C for long-term storage.

PHARMALINE®

RUO

Malaria Detection Kit **Cat No: PHMLR2022 100**

Validation Data

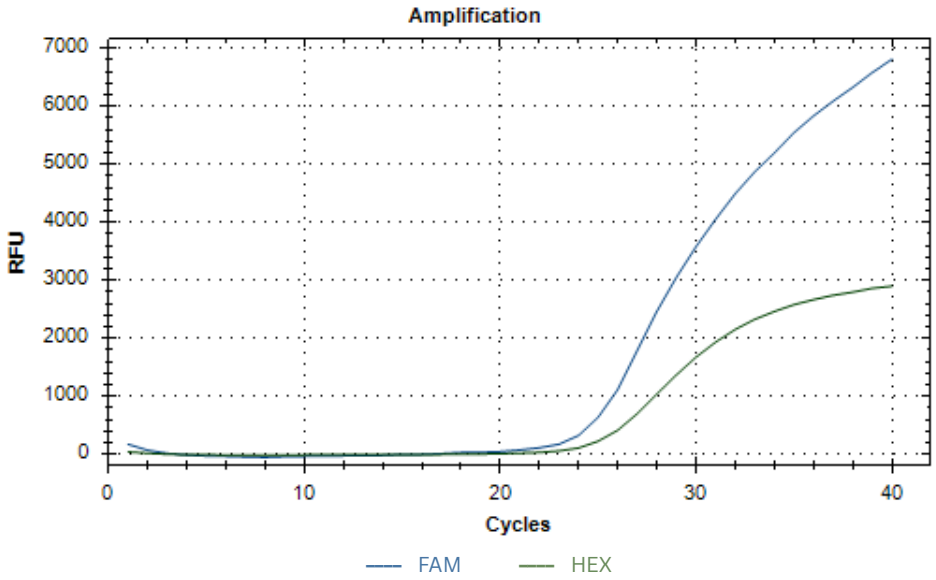


Figure 1. **Positive Amplification Profile:** The plot demonstrates a specific signal increase exceeding the threshold in the target channel (FAM: Plasmodium spp. - all species). Positivity detected in the target channel is diagnostically valid, regardless of the HEX (Internal Control) signal.

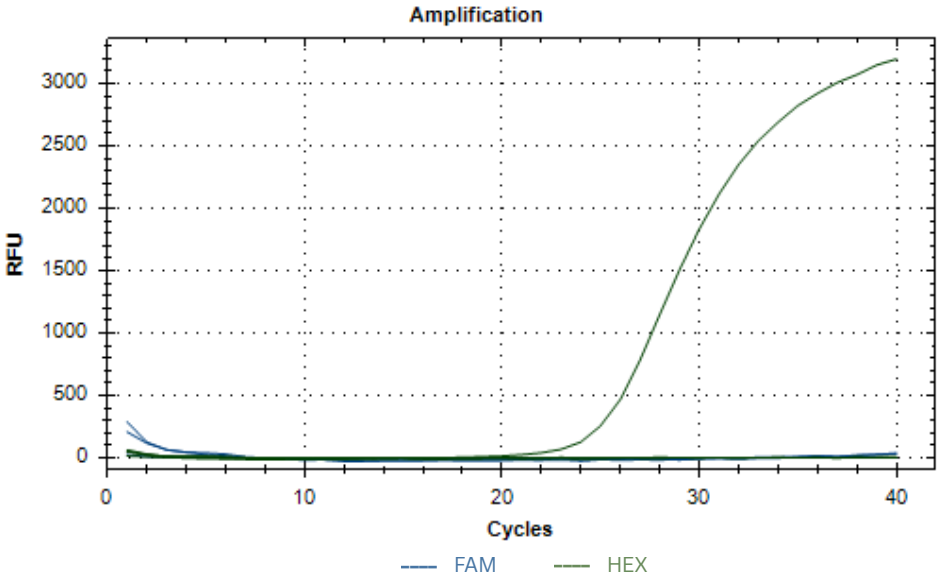


Figure 2. **Negative Amplification Profile:** No specific signal increase was detected in the target channel (FAM). Analytical validity and sample integrity are confirmed by the positive signal in the HEX (Internal Control) channel. If both channels remain negative, the test is considered invalid and must be repeated.

Xplogen

RUO

Xplogen SMA qPCR Screening Kit **Cat No: PHSMA2024 100/1000**

Product Overview and Targets

The Xplogen SMA qPCR Screening Kit is an in vitro diagnostic tool designed for the detection of Spinal Muscular Atrophy (SMA). SMA is an autosomal recessive disease caused by mutations in the SMN1 (Survival Motor Neuron) gene. Approximately 95% of SMA patients lack both copies of SMN1 exon 7.

This kit utilizes Quantitative Real Time PCR (qPCR) to detect the C/T change at the 840th nucleotide of SMN1 Exon 7, distinguishing it from the SMN2 gene. It works on the principle of Copy Number Variation (CNV) analysis using the ΔΔCt method.

Detected Targets and Genotyping

This kit performs the detection of autosomal recessive SMA disease using 4-channel qPCR instruments, utilizing two primary channels for analysis:

- FAM Channel Target: SMN1 Exon 7 (Target Gene for Deletion Status detection)
- HEX Channel Target: Human Actin-β gene (Internal Reference Gene for normalization)

The kit determines copy number variation (CNV) based on the ΔΔCt method to classify the genotype:

- Non-carrier: ΔΔCt> 0.5 (2 copies Exon 7)
- Carrier/Heterozygous: 0.01-0.5 (1 copy Exon 7)
- Patient/Homozygous Deletion: 0-0.01 (0 copies Exon 7)

Key Features

- Dedicated Analysis **Software**: The kit is supported by **proprietary software** for automated ΔΔCt calculation and highly accurate result interpretation.
- High Performance: Designed to achieve a minimum of 98% specificity and 98% sensitivity.
- Sample Type: Applied to genomic DNA isolated from Whole Blood samples of individuals suspected of being carriers.
- CNV Analysis: Provides quantitative copy number determination of the SMN1 Exon 7 deletion.
- Reliability: Includes Negative Control (NTC) and Positive Control (PC) for contamination and reagent stability control.
- Certification: CE IVD marked and strictly for professional in vitro diagnostic use only.

Technical Details and Storage

- Kit Components: Contains 2X Master Mix (DNA polymerase, dNTP mix, ribonuclease inhibitor) and Primer Mix (SMN1 Exon 7 and Human Actin-β specific probes).
- Storage Temperature: Stable between (-15°C) and (-25°C)
- Shelf Life: 12 months.

Xplogen

RUO

Xplogen SMA qPCR Screening Kit **Cat No: PHSMA2024 100/1000**

Validation Data

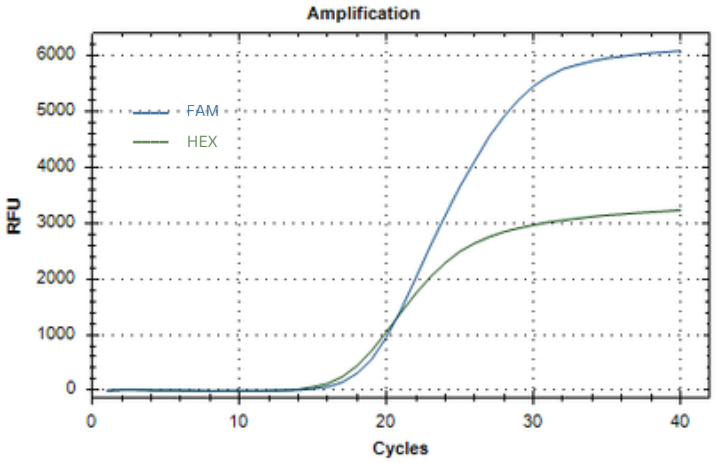


Figure 1. **Healthy Genotype Profile:** The plot demonstrates strong amplification in both the FAM (SMN1 Exon 7) and HEX (Actin-β) channels. A ΔΔCt Ct > 0.5 confirms the presence of two SMN1 copies, indicating a healthy genotype.

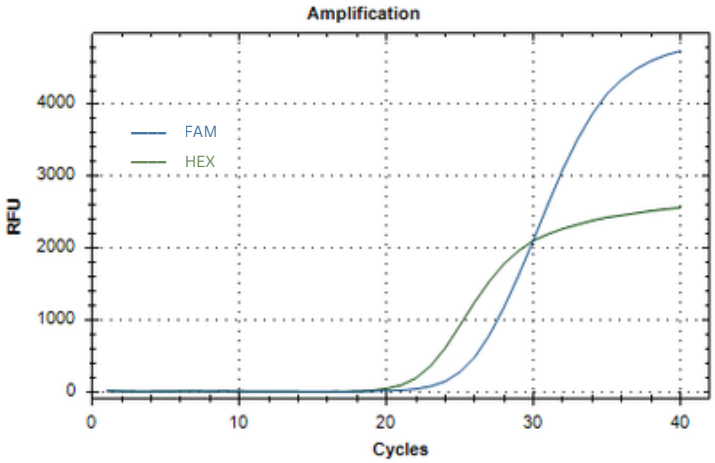


Figure 2. **Carrier (Heterozygous) Profile:** The plot reflects a single-copy deletion of SMN1. While the HEX (Actin-β) channel amplifies normally, the FAM channel shows a delayed signal. A ΔΔCt value between 0.01 and 0.5 classifies the individual as an SMA carrier.

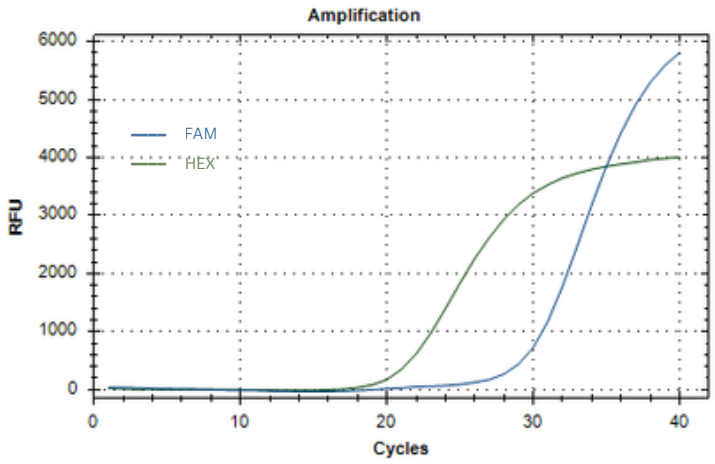



Figure 3. **Patient (Homozygous Deletion) Profile:** The plot shows a complete absence of SMN1 Exon 7 amplification in the FAM channel, while the HEX (Actin-β) channel remains positive for normalization. A ΔΔCt value between 0 and 0.01 confirms an SMA diagnosis.

PHARMALINE

ONCOLOGY | MICROBIOLOGY | MEDICAL GENETICS

PHARMALINE

ONCOLOGY | MICROBIOLOGY | MEDICAL GENETICS

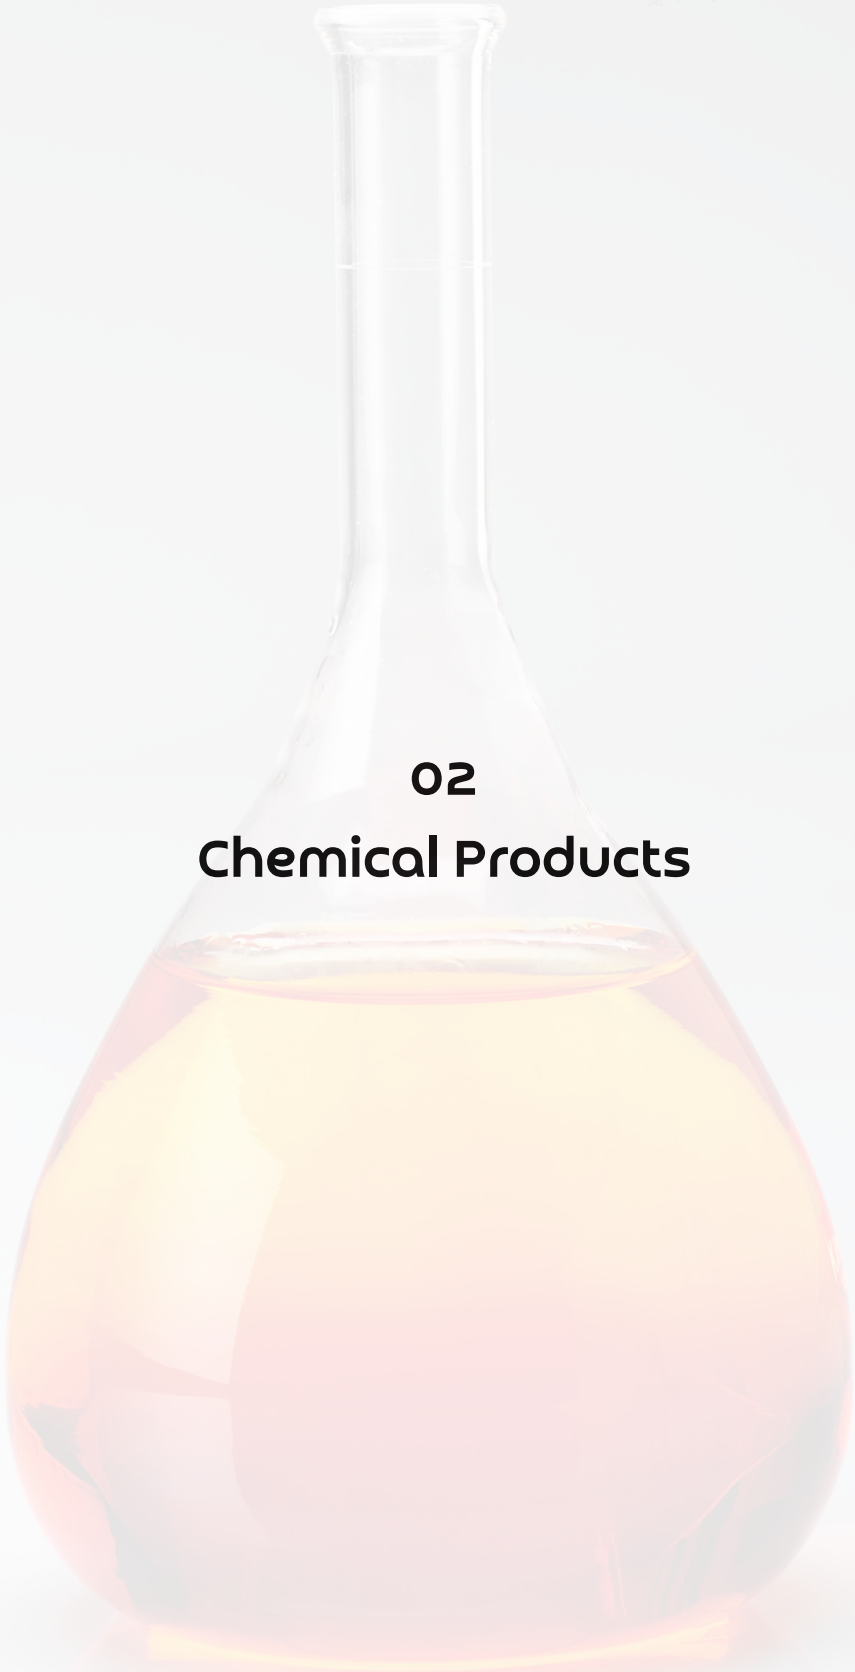

02

Chemical Products

PHARMASEP

RUO

Stool Extraction Preparation Buffer — Cat No: PHSP2024 50/100

Product Overview

PharmaSEP is a versatile buffer solution designed primarily as a Stool Extraction Preparation Buffer for in vitro diagnostic use. It has a wide range of uses in biological and biochemical research.


Key Features

- Versatile Use: A reliable tool for pH stabilization, providing an isotonic environment, cleaning nucleic acids during isolation, and the preparation/dilution of biological reagents.
- Reliable Sample Prep: Ensures reliable and standardized preparation of nucleic acid extracts from challenging stool sample.
- Convenient Storage: Can be stored and transported at room temperature, between 15°C and 25°C.
- Shelf Life: 12 months.


Stool Sample Preparation Protocol Highlights

The buffer facilitates a simple preparation process for extraction:


1. Mixing: The stool sample (100 mg solid or 100 µl liquid) is added to 900 µl of PharmaSEP and vortexed at the highest speed for 30 seconds.
2. Freezing: The mixture is frozen at -20°C for 30 minutes.
3. Centrifugation: After thawing, the sample is centrifuged at 5000g for 15 minutes.
4. Extraction Ready: The resulting supernatant is then ready for nucleic acid extraction.

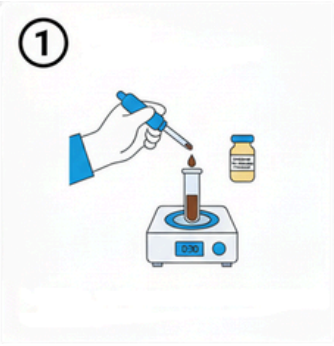


1. Mixing:
100 mg stool + 900 µl PharmaSEP, vortex for 30 sec.

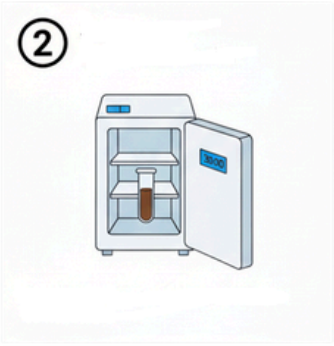

2. Freezing:
The mixture is frozen at -20°C for 30 min.

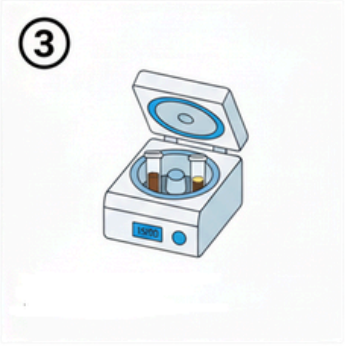

3. Centrifugation:
5000 g for 15 minutes.

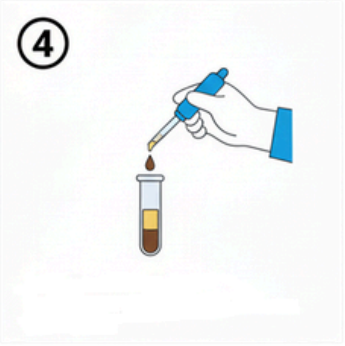

4. Extraction Ready:
Supernatant is ready for nucleic acid extraction.

PHARMALINE®

RUO

PharmaDirect qPCR Solüsyonu **Cat No: PHSP2024 50/100**

Product Overview and Targets

The PharmaDirect qPCR Solution is designed to allow clinical samples contained within Viral Transport Medium (VTM) to be used directly in qPCR assays without the need for any nucleic acid purification process.

Its special formulation ensures that viral pathogens present in the VTM are lysed (disrupted) during the pre-denaturation step of the PCR reaction, leading to the release of nucleic acid. The specialized chemicals stabilize the released nucleic acid, prevent non-specific binding during amplification, and enhance amplification efficiency.

Key Features

- Extraction-Free qPCR: Eliminates the nucleic acid extraction step, significantly reducing hands-on time and costs.
- Enhanced Efficiency: Special chemicals stabilize the nucleic acid and prevent non-specific binding, improving amplification yield.
- Compatibility: Optimized for use with Pharmaline brand qPCR kits for optimal results.
  - Note on Limitations: The solution is developed for DNA viruses and is not suitable for use with RNA viruses.
  - The elimination of the extraction step may increase the protein contamination rate in PCR wells, potentially reducing the sensitivity of the qPCR kit by 1–2%.
- Reaction Composition (Example): A typical 15 µl Direct qPCR Reaction Mix includes 7.5 µl of 2X Master Mix (resulting in a 1X final concentration), 2.5 µl of Primer Mix, 2.5 µl of PharmaDirect Solution, and 2.5 µl of VTM Sample.

Technical Details and Storage

- Storage Conditions: Store and transport at room temperature (below 25°C) with the lid tightly closed.
- pH Sensitive: The solution is pH-adjusted and can be affected by ambient gases; ensure the solution is not exposed to air during storage.
- Handling: Gently mix the master mix, primer mix, and PharmaDirect solution by inverting them (do not vortex) to homogenize the mixture before dispensing.
- UV Protection: Protect the solution from Ultraviolet (UV) light.

PharmaLine Healthcare Services Industry and Trade Inc.

🏢 Atatürk Street, Atatürk Residences No:43, Block A, Apartment 6, Sahrayıcedit Neighborhood, Kadıköy/Istanbul, Türkiye

🏭 Gersan Industrial Site, 2308th Street No:52, Yenimahalle/Ankara, Türkiye

📞 +90 (216) 346 86 66

📩 info@pharmaline.com.tr